

Mid-infrared laser phase-locking to a remote near-infrared frequency reference for high-precision molecular spectroscopy

B Chanteau, O. Lopez, W Zhang, D Nicolodi, B Argence, F Auguste, M Abgrall, C Chardonnet, G Santarelli, B Darquié, et al.

► **To cite this version:**

B Chanteau, O. Lopez, W Zhang, D Nicolodi, B Argence, et al.. Mid-infrared laser phase-locking to a remote near-infrared frequency reference for high-precision molecular spectroscopy. *New Journal of Physics*, Institute of Physics: Open Access Journals, 2013, 15, pp.073003. <10.1088/1367-2630/15/7/073003>. <hal-01587027>

HAL Id: hal-01587027

<http://hal.upmc.fr/hal-01587027>

Submitted on 13 Sep 2017

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



PAPER • OPEN ACCESS

Mid-infrared laser phase-locking to a remote near-infrared frequency reference for high-precision molecular spectroscopy

To cite this article: B Chanteau *et al* 2013 *New J. Phys.* **15** 073003

View the [article online](#) for updates and enhancements.

Related content

- [Topical Review](#)
P Maddaloni, P Cancio and P De Natale
- [Measurement of optical frequencies and frequency ratios](#)
Harald Schnatz
- [Ultra-stable long distance optical frequency distribution using the Internet fiber network and application to high-precision molecular spectroscopy](#)
O Lopez, B Chanteau, A Bercy *et al.*

Recent citations

- [Characterising molecules for fundamental physics: an accurate spectroscopic model of methyltrioxorhenium derived from new infrared and millimetre-wave measurements](#)
Pierre Asselin *et al*
- [In-field Raman amplification on coherent optical fiber links for frequency metrology](#)
C. Clivati *et al*
- [Stable low noise 1.5 \$\mu\text{m}\$ laser generated by a singly resonant optical parametric oscillator](#)
Li Peng *et al*

Mid-infrared laser phase-locking to a remote near-infrared frequency reference for high-precision molecular spectroscopy

B Chanteau¹, O Lopez¹, W Zhang², D Nicolodi², B Argence¹, F Auguste¹, M Abgrall², C Chardonnet¹, G Santarelli^{2,3}, B Darquié¹, Y Le Coq² and A Amy-Klein^{1,4}

¹Laboratoire de Physique des Lasers, Université Paris 13, Sorbonne Paris Cité, CNRS, 99 Avenue Jean-Baptiste Clément, F-93430 Villetaneuse, France

²LNE-SYRTE, Observatoire de Paris, CNRS, UPMC, 61 Avenue de l'Observatoire, F-75014 Paris, France

³Laboratoire Photonique, Numérique et Nanosciences, Université de Bordeaux 1, Institut d'Optique and CNRS, 351 cours de la Libération, F-33405 Talence, France

E-mail: amy@univ-paris13.fr

New Journal of Physics **15** (2013) 073003 (10pp)

Received 14 April 2013

Published 2 July 2013

Online at <http://www.njp.org/>

doi:10.1088/1367-2630/15/7/073003

Abstract. We present a method for accurate mid-infrared frequency measurements and stabilization to a near-infrared ultra-stable frequency reference, transmitted with a long-distance fibre link and continuously monitored against state-of-the-art atomic fountain clocks. As a first application, we measure the frequency of an OsO₄ rovibrational molecular line around 10 μm with an uncertainty of 8×10^{-13} . We also demonstrate the frequency stabilization of a mid-infrared laser with fractional stability better than 4×10^{-14} at 1 s averaging time and a linewidth below 17 Hz. This new stabilization scheme gives us the ability to transfer frequency stability in the range of 10^{-15} or even better, currently accessible in the near infrared or in the visible, to mid-infrared lasers in a wide frequency range.

⁴ Author to whom any correspondence should be addressed.



Content from this work may be used under the terms of the [Creative Commons Attribution 3.0 licence](http://creativecommons.org/licenses/by/3.0/). Any further distribution of this work must maintain attribution to the author(s) and the title of the work, journal citation and DOI.

Contents

1. Introduction	2
2. Experimental setup	3
3. Mid-infrared frequency measurement and stabilization	5
4. Conclusion	7
Acknowledgments	8
References	8

1. Introduction

With their rich internal structure, molecules can play a decisive role in precision tests of fundamental physics. They are, for example, now being used to test fundamental symmetries [1–3] and to measure either absolute values of fundamental constants [4] or their temporal variation [5–6]. Most of those experiments can be cast as the measurement of molecular frequencies. Ultra-stable and accurate sources in the mid-infrared (MIR) spectral region, the so-called molecular fingerprint region that hosts many intense rovibrational signatures, are thus highly desirable. MIR laser frequency stabilization has been performed for a long time using molecular references such as CH₄ or OsO₄ (see for instance [7–10]). However obtained stability is at least one order of magnitude below those of visible or near-infrared lasers stabilized to an ultra-stable cavity. Moreover, only a few molecular lines can be used when ultra-high accuracy is needed.

In this paper we present a method for accurate MIR laser frequency stabilization. The frequency reference is a near-infrared cavity-stabilized laser continuously monitored against primary standards, and the coherent frequency link between near-infrared and MIR frequencies is obtained by using an optical frequency comb. Moreover, we demonstrate this stabilization scheme with a remote near-infrared frequency reference transferred via an optical fibre link from a national metrological institute (NMI). This technique is thus accessible to any laboratory that can be connected to such an NMI with a fibre optical link [11].

Optical frequency combs have proven to be essential for laser frequency measurement and stabilization from the infrared to ultraviolet domain (see for instance [12]). Fractional accuracy and stability (at 1 day averaging time) down to a few 10^{-16} are potentially reachable when the frequency reference is provided by advanced primary standards. Extension to the MIR spectral domain has been demonstrated by comparing the MIR laser frequency with a very high harmonic of the comb repetition rate using sum-frequency generation (SFG) or difference-frequency generation [13–20]. Efforts have also been made towards the development of MIR frequency combs [10, 21–26].

In this paper we first describe the setup for coherent frequency stability transfer between near-infrared and MIR frequencies around $10\ \mu\text{m}$. Then we demonstrate absolute frequency measurement of a MIR frequency with a fractional resolution of at least 4×10^{-14} . We also report a first application to high-resolution molecular spectroscopy with a fractional uncertainty of 8×10^{-13} on the line centre. Finally, we present the MIR laser frequency stabilization against the near-infrared frequency reference.

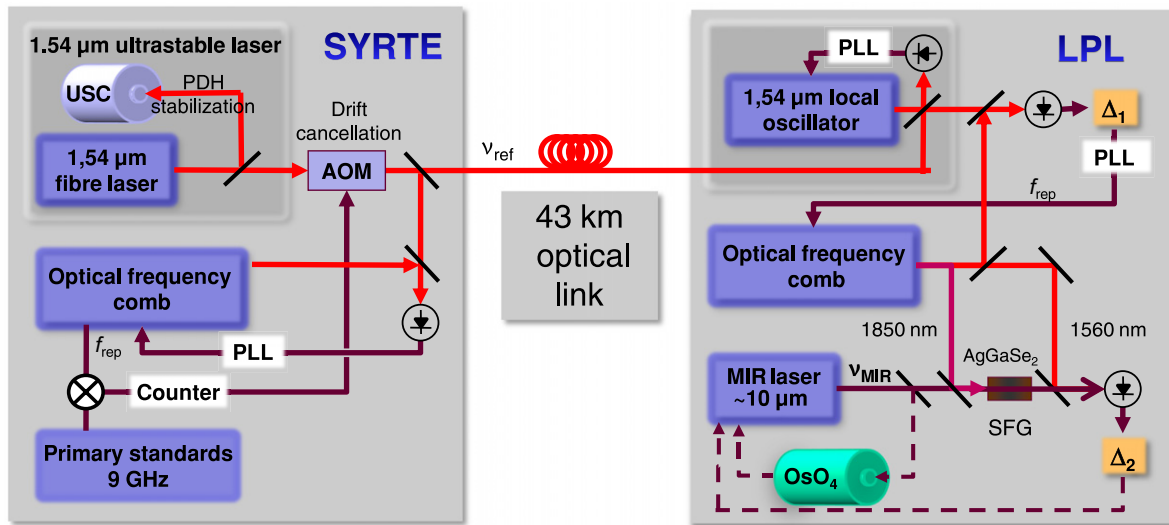


Figure 1. Experimental setup. The MIR laser frequency can be controlled with either the beat-note Δ_2 or the OsO_4 absorption signal. PLL: phase-lock loop; PDH: Pound–Drever–Hall stabilization; SFG: sum-frequency generation; AOM: acousto-optic modulator; USC: ultra-stable cavity.

2. Experimental setup

The experimental setup is shown in figure 1. The ultra-stable optical reference located at LNE-SYRTE is a $1.54\ \mu\text{m}$ fibre laser locked to a high-finesse cavity. Its fractional frequency instability was measured to be lower than 2×10^{-15} at 1 s and 10^{-14} at 100 s (after a $0.3\ \text{Hz s}^{-1}$ drift was removed) [27]. Its frequency is measured using a fibre fs laser centred around $1.55\ \mu\text{m}$. The laser repetition rate is phase-locked to the optical reference frequency after removal of the comb frequency offset f_0 . Fast corrections are applied to an intra-cavity electro-optic modulator (bandwidth $>400\ \text{kHz}$) and slower corrections to a piezo-electric transducer (PZT) controlling the laser cavity length (bandwidth $\sim 10\ \text{kHz}$) [28]. The absolute frequency of the comb repetition rate 36th harmonic (9 GHz) is continuously measured against the LNE-SYRTE frequency references, which includes an H-maser, a cryogenic oscillator and Cs fountains [29–30]. It enables real-time measurement of the ultra-stable laser frequency drift and its correction by applying to the driving frequency of an acousto-optic modulator an opposite linear drift (with a step every ms) updated every 100 s. This makes up an ultra-stable near-infrared reference, the frequency of which is currently traceable to primary standards with a 10^{-14} uncertainty after 100 s.

This optical reference signal is transmitted to Laboratoire de Physique des Lasers (LPL) through a 43 km long optical link [27]. The free-running link exhibits a propagation instability of 2×10^{-14} at 1 s and around 10^{-15} between 100 s and 1 day. When compensated, the link instability has been measured to be roughly $10^{-15}\ \tau^{-1}$ and to reach around 10^{-18} after 10^3 s (see figure 3) [27]. The frequency stability and accuracy of the reference signal are thus preserved at the LPL optical link end.

At LPL, a low-noise laser diode (free-running linewidth below 10 kHz) is phase-locked to the incoming signal with a bandwidth of 100 kHz and constitutes the local optical frequency

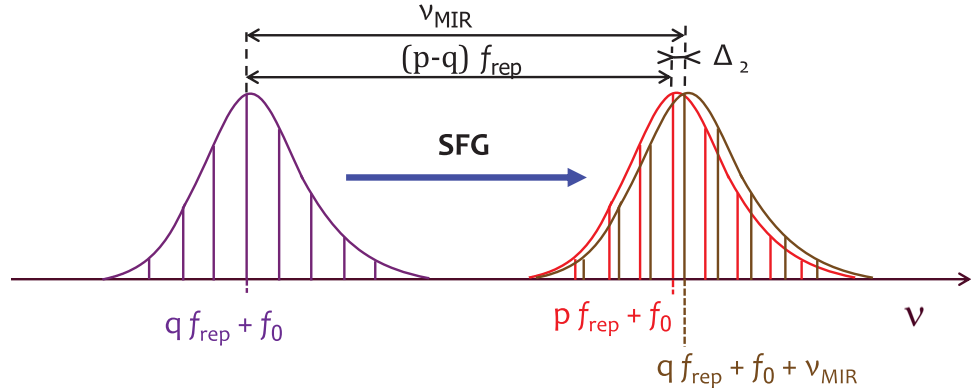


Figure 2. Sum-frequency of a comb output centred at 1850 nm (purple comb), of mode frequencies $qf_{\text{rep}} + f_0$ with q an integer, and the MIR laser (of frequency ν_{MIR} around 10 μm) results in a shifted comb (brown comb) centred at 1550 nm of mode frequencies $qf_{\text{rep}} + f_0 + \nu_{\text{MIR}}$. The beat-note of this shifted comb with the comb main output centred at 1550 nm (red comb), of mode frequencies $pf_{\text{rep}} + f_0$ with p an integer, can be written as $\Delta_2 = \pm((qf_{\text{rep}} + f_0 + \nu_{\text{MIR}}) - (pf_{\text{rep}} + f_0))$, which results in $\Delta_2 = \pm(\nu_{\text{MIR}} - (p - q)f_{\text{rep}})$. SFG: sum-frequency generation.

reference ν_{ref} . The repetition rate f_{rep} of a 1.55 μm fibre fs laser is phase-locked to ν_{ref} . To that purpose, the beat-note Δ_1 between ν_{ref} and the N th comb mode ($N \sim 780\,000$) is used, after removal of the comb frequency offset f_0 :

$$\nu_{\text{ref}} - N f_{\text{rep}} = \pm \Delta_1. \quad (1)$$

Fast and slow corrections are applied to an intra-cavity electro-optic modulator and a PZT, respectively, as performed at LNE-SYRTE [28]. A second beat-note Δ_2 compares the MIR laser frequency ν_{MIR} around 10 μm and the n th harmonic of the repetition rate with $n \approx 120\,000$:

$$\nu_{\text{MIR}} - n f_{\text{rep}} = \pm \Delta_2. \quad (2)$$

This signal is generated using SFG of the MIR light and an additional comb output centred on 1.85 μm , generated in a nonlinear fibre (figure 2) [14]. This comb output (~ 25 mW) and the MIR laser beam (~ 100 mW) are focused in a 10 mm long crystal of AgGaSe₂ for type-I SFG. The measured efficiency is around 0.4 mW/W² and the phase-matching bandwidth (for the 1.85 μm comb) is about 30 nm (~ 3 THz). The resulting shifted comb, centred on 1.55 μm , is combined with the 1.55 μm fs laser output. An adjustable delay line enables us to control the overlapping of the pulses in the time domain. About 10^4 mode pairs generate the beat-note Δ_2 which shows a signal-to-noise ratio of about 30 dB in a 100 kHz bandwidth. An RF tracking oscillator is phase-locked to this beat-note. As a result of the frequency difference between two modes of the same comb, Δ_2 is independent of the comb offset f_0 .

Combining (1) and (2), the MIR laser frequency ν_{MIR} is finally obtained as

$$\nu_{\text{MIR}} = \pm \Delta_2 + \frac{n}{N} (\nu_{\text{ref}} \mp \Delta_1) \quad (3)$$

with n/N roughly equal to 0.15. The MIR frequency is thus directly linked to the near-infrared frequency reference, once the integers n and N and the signs have been determined.

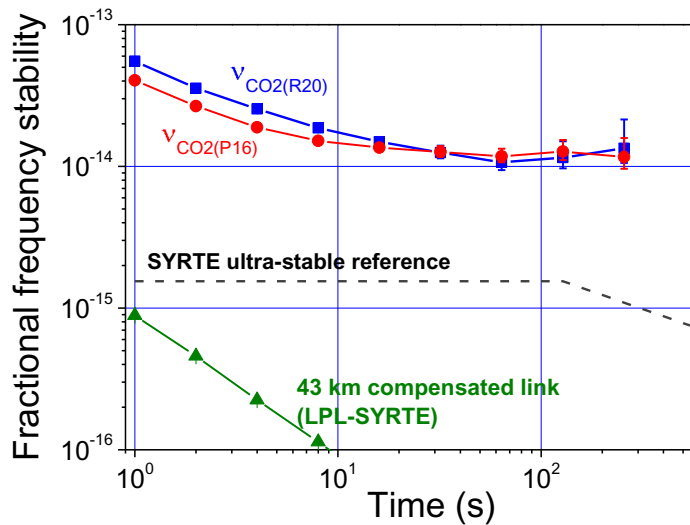


Figure 3. Frequency stability of a CO₂ laser locked on two different OsO₄ saturated absorption lines: the P(55) line of ¹⁹⁰OsO₄ near the 10.55 μm P(16) CO₂ laser line (red circles ●) and the R(67) line of ¹⁹²OsO₄ near the 10.25 μm R(20) CO₂ laser line (blue squares ■). The propagation instability of the compensated LPL-SYRTE fibre link (green up-triangles ▲) and the stability of the SYRTE frequency reference that is made of a combination of an H-maser, a cryogenic oscillator and Cs fountains [29] (dashed line) are shown for comparison.

3. Mid-infrared frequency measurement and stabilization

To characterize the phase-coherent link between the near-infrared frequency reference and the MIR frequency, we used this setup to measure the absolute frequency of a CO₂ laser stabilized onto an OsO₄-saturated absorption line. Such an OsO₄-stabilized CO₂ laser constitutes the current state-of-the-art MIR secondary reference standard [7, 8]. In this work, the CO₂ laser was locked either to the P(55) line of ¹⁹⁰OsO₄ near the 10.55 μm P(16) CO₂ laser line or to the R(67) line of ¹⁹²OsO₄ near the 10.25 μm R(20) CO₂ laser line. Corrections are applied to a PZT controlling the laser cavity length with a stabilization bandwidth of about 400 Hz limited by the PZT actuator. The obtained fractional frequency stability, shown in figure 3 (red circles and blue squares), is 4×10^{-14} at 1 s, reaches 10^{-14} after 100 s of integration, and degrades at longer times due to a frequency drift of the CO₂/OsO₄ frequency reference. We checked that this stability was limited by the CO₂/OsO₄ reference since changing the CO₂ laser locking parameters induced a variation of the obtained stability. This stability is consistent with previous measurements obtained by comparing either two identical stabilized CO₂ lasers [7–8] or one of such lasers to a titanium–sapphire (Ti:Sa) frequency comb referenced to a microwave frequency [13]. This demonstrates the capability of the system to measure the stability of the best MIR frequency sources to date without any degradation. We expect the optical link and the frequency comb to contribute a few 10^{-15} at 1 s to the frequency instability [27–28].

The relationship of equation (3) between the frequency of the 1.54 μm LNE-SYRTE reference laser and that of the MIR laser is ensured by means of coherent phase-lock loops.

Thus the accuracy of the MIR frequency measurement only depends on the uncertainty of the near-infrared frequency reference. The latter is known with an uncertainty of about 10^{-14} after 100 s averaging time, when only steered with the H-maser which is sufficient for this experiment. The 3×10^{-16} Cs fountain accuracy [30] can ultimately be reached and then transferred from the optical reference to the MIR frequency.

As a first application to high-precision spectroscopy, we determined the absolute frequency of the P(55) line of $^{190}\text{OsO}_4$ by measuring the OsO_4 -stabilized CO_2 laser frequency. Eleven measurements were performed between December 2011 and April 2012. The beat-note Δ_2 , the repetition rate f_{rep} and the frequency ν_{ref} were counted with a gate time of 1 s. Δ_2 and ν_{ref} were combined using equation (3) to calculate the CO_2/OsO_4 frequency. Signs in equation (3) and values of n and N were unambiguously deduced from f_{rep} and the value $\nu_{\text{OsO}_4/1999} = 28\,412\,648\,819\,596(45)$ Hz of the CO_2/OsO_4 frequency obtained by combining two independent measurements reported in the literature [31, 32]. The mean value over 600 measurements of 1 s of the CO_2/OsO_4 frequency gives one data point. For each data point, we correct the frequency of the LNE-SYRTE H-maser using the data published by Bureau International des Poids et Mesures⁵. Between each measurement the OsO_4 absorption cell was pumped and filled again or the whole experiment was switched off and on. We obtained $\nu_{\text{OsO}_4/2012} = 28\,412\,648\,819\,588(24)$ Hz where the uncertainty is the weighted $1 - \sigma$ deviation of the data points. It is -8 Hz from the value $\nu_{\text{OsO}_4/1999}$ and $+8$ Hz from another measurement performed in 2004 with a microwave-referenced Ti:Sa frequency comb with an uncertainty of 58 Hz [13]. Within $1 - \sigma$ error bars the present result agrees with the previous measurements and confirms the very high accuracy of the measurement setup. The factor of 2 improvement of the uncertainty obtained in the measurement reported here, still limited by the molecular reference, is due to a better control of the OsO_4 pressure and optimization of the CO_2 laser locking parameters.

From the previous results, we conclude that the coherent frequency chain is a viable and potentially much better alternative to an OsO_4 molecular transition for frequency stabilization of a MIR source. This was investigated by locking the CO_2 laser frequency to the optical comb: the beat-note of the free-running CO_2 laser with the comb repetition rate n th harmonic, Δ_2 , was phase-locked onto a stable frequency synthesizer with a 400 Hz bandwidth. The obtained CO_2 laser frequency stability is characterized by measuring the beat-note Δ_3 with a second independent CO_2 laser stabilized onto OsO_4 . Figure 4 displays this beat-note signal, fitted with a Lorentzian of linewidth 17 Hz (full-width at half-maximum). In the case of a Lorentzian lineshape, the contribution of each laser linewidth adds [33] and we deduce a linewidth between 8.5 and 17 Hz for each laser, the state of the art for a CO_2 laser [7]. Figure 5 displays Δ_3 's frequency noise power spectral density (PSD) (red trace). Using the beat-note Δ_2 with the local frequency comb, the frequency noise PSD of the OsO_4 -stabilized CO_2 laser was also measured (figure 5, blue trace). The two PSDs almost perfectly overlap as expected from efficient phase stabilization. Together with the above results, it shows that the comb-stabilized MIR laser frequency noise is at least as low as that of the OsO_4 -stabilized laser. The former is most probably much lower, potentially compatible with the frequency noise of the optical frequency reference of which the inferred PSD (including noise added by the link) is displayed in figure 5 (dotted black line). This noise level is the lowest reachable with our stabilization scheme.

⁵ See publication of the clocks' rates relative to TAI on [ftp://ftp2.bipm.org/pub/tai/publication/](http://ftp2.bipm.org/pub/tai/publication/).

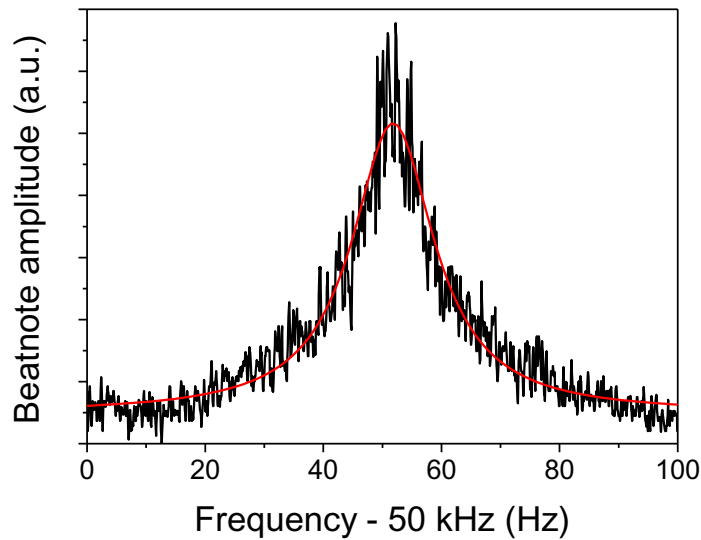


Figure 4. Down-converted beat-note of two independent CO₂ lasers, one stabilized on an OsO₄ resonance line, the other phase-locked to a comb repetition rate high-harmonic; the red line is a Lorentzian fit of linewidth 17 Hz.

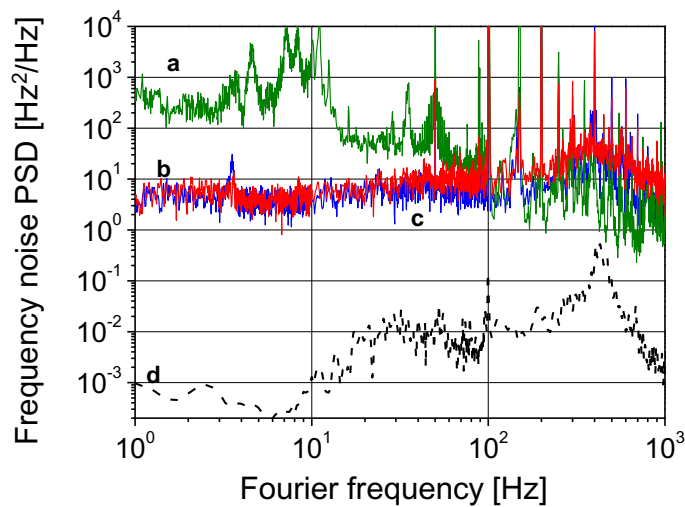


Figure 5. Frequency noise PSD of (a) the free-running CO₂ laser (green trace), (b) the beat-note between the CO₂ laser stabilized onto the frequency comb and an independent OsO₄-stabilized CO₂ laser (red trace), (c) the OsO₄-stabilized CO₂ laser measured with the comb (blue trace) and (d) the optical reference (dotted black line). The free-running CO₂ laser PSD has been measured using the beat-note Δ_2 with the local frequency comb and is given for comparison.

4. Conclusion

We have demonstrated a coherent frequency chain linking a remote ultra-stable 1.54 μm frequency reference and a MIR source, leading to the control of the absolute MIR frequency.

It uses reliable commercially available fibre-based frequency combs and an optical reference potentially available to any laboratory connected to a fibre network [11]. Stability below 4×10^{-14} at 1 s was demonstrated, and we expect it to be in the 10^{-15} range. Using a state-of-the-art near-infrared ultra-stable laser [34] may reduce this value even further. The 3×10^{-16} accuracy of the LNE-SYRTE Cs fountains is potentially within reach.

Frequency tuning of such a stabilized MIR laser source, required for high-resolution spectroscopy, is achievable by scanning the near-infrared frequency referencing the comb. Tuning the frequency offset between the LNE-SYRTE optical reference and the LPL laser diode of frequency ν_{ref} (see equation (3)) would result in a tuning range of a few GHz.

This setup enables us to stabilize MIR laser sources in a much wider spectral range than is currently possible using the OsO₄ molecular standard. With the present setup the 9–11 μm range is accessible, limited by the nonlinear crystal and the central frequency of the auxiliary 1.85 μm comb output used in the SFG. Nevertheless, it can easily be extended to the whole 5–20 μm range with the proper comb spectrum and crystal optimization. Orientation-patterned GaAs would for instance ensure a wide tunability [35]. Our stabilization technique is thus particularly well suited to quantum cascade lasers that have achievable wavelengths covering the whole MIR region [36]. Moreover, the ongoing work on dissemination of optical reference through internet fibre networks over a continental scale [11] will eventually enable many laboratories to access an ultra-stable optical reference. Thus such ultra-stable and accurate MIR sources could benefit a very wide molecular spectroscopy community.

Acknowledgments

The authors acknowledge financial support from CNRS, Agence Nationale de la Recherche (ANR BLANC 2011-BS04-009-01) and Université Paris 13. Sylvain Dimanno is gratefully acknowledged for contributing to the comb driving software.

References

- [1] DeMille D, Cahn S B, Murphree D, Rahmlow D A and Kozlov M G 2008 Using molecules to measure nuclear spin-dependent parity violation *Phys. Rev. Lett.* **100** 023003
- [2] Darquié B *et al* 2010 Progress toward a first observation of parity violation in chiral molecules by high-resolution laser spectroscopy *Chirality* **22** 870–84
- [3] Hudson J J, Kara D M, Smallman I J, Sauer B E, Tarbutt M R and Hinds E A 2011 Improved measurement of the shape of the electron *Nature* **473** 493–6
- [4] Koelemeij J C J, Roth B, Wicht A, Ernsting I and Schiller S 2007 Vibrational spectroscopy of HD⁺ with 2-ppb accuracy *Phys. Rev. Lett.* **98** 173002
- [5] Shelkownikov A, Butcher R J, Chardonnet C and Amy-Klein A 2008 Stability of the proton-to-electron mass ratio *Phys. Rev. Lett.* **100** 150801
- [6] Hudson E R, Lewandowski H J, Sawyer B C and Ye J 2006 Cold molecule spectroscopy for constraining the evolution of the fine structure constant *Phys. Rev. Lett.* **96** 143004
- [7] Bernard V, Daussy C, Noguees G, Constantin L, Durand P E, Amy-Klein A, van Lerberghe A and Chardonnet C 1997 CO₂ laser stabilization to 0.1 Hz level using external electrooptic modulation *IEEE J. Quantum Electron.* **33** 1282–7
- [8] Acef O 1997 Metrological properties of CO₂/OsO₄ optical frequency standard *Opt. Commun.* **134** 479–86

- [9] Gubin M A, Tyurikov D A, Shelkovnikov A S, Koval'chuk E V, Kramer G and Lipphardt B 1995 Transportable HeNe/CH₄ optical frequency standard and absolute measurements of its frequency *IEEE J. Quantum Electron.* **31** 2177–82
- [10] Foreman S M, Marian A, Jun Ye J, Petrukhin E A, Gubin M A, Mücke O D, Wong F N C, Ippen E P and Kärtner F X 2005 Demonstration of a HeNe/CH₄-based optical molecular clock *Opt. Lett.* **30** 570–2
- [11] Lopez O, Haboucha A, Chanteau B, Chardonnet C, Amy-Klein A and Santarelli G 2012 Ultra-stable long distance optical frequency distribution using the internet fiber network *Opt. Express* **20** 23518–26
- [12] Cundiff S T, Ye J and Hall J L 2001 Optical frequency synthesis based on mode-locked lasers *Rev. Sci. Instrum.* **72** 3749–71
- [13] Daussy C *et al* 2005 Long-distance frequency dissemination with a resolution of 10⁻¹⁷ *Phys. Rev. Lett.* **94** 203904
- [14] Amy-Klein A, Goncharov A, Guinet M, Daussy C, Lopez O, Shelkovnikov A and Chardonnet C 2005 Absolute frequency measurement of a SF₆ two-photon line by use of a femtosecond optical comb and sum-frequency generation *Opt. Lett.* **30** 3320–2
- [15] Bielsa F, Djerroud K, Goncharov A, Douillet A, Valenzuela T, Daussy C, Hilico L and Amy-Klein A 2008 HCOOH high resolution spectroscopy in the 9.18 μm region *J. Mol. Spectrosc.* **247** 41–6
- [16] Vainio M, Merimaa M and Halonen L 2012 Frequency-comb-referenced molecular spectroscopy in the mid-infrared region *Opt. Lett.* **36** 4122–4
- [17] Bressel U, Ernsting I and Schiller S 2012 5 μm Laser source for frequency metrology based on difference frequency generation *Opt. Lett.* **37** 918–20
- [18] Borri S *et al* 2012 Direct link of a mid-infrared QCL to a frequency comb by optical injection *Opt. Lett.* **37** 1011–3
- [19] Mills A A, Gatti D, Jiang J, Mohr C, Mefford W, Gianfrani L, Fermann M, Hartl I and Marangoni M 2012 Coherent phase lock of a 9 μm quantum cascade laser to a 2 μm thulium optical frequency comb *Opt. Lett.* **37** 4083–5
- [20] Galli I *et al* 2013 Comb-assisted subkilohertz linewidth quantum cascade laser for high-precision mid-infrared spectroscopy *Appl. Phys. Lett.* **102** 121117
- [21] Schliesser A, Picqué N and Haensch T W 2012 Mid-infrared frequency combs *Nature Photon.* **6** 440–9
- [22] Adler F, Cossel K C, Thorpe M J, Hartl I, Fermann M E and Ye J 2009 Phase-stabilized, 1.5 W frequency comb at 2.8–4.8 μm *Opt. Lett.* **34** 1330–2
- [23] Baumann E, Giorgetta F R, Swann W C, Zolot A M, Coddington I and Newbury N R 2011 Spectroscopy of the methane ν_3 -band with an accurate midinfrared coherent dual-comb spectrometer *Phys. Rev. A* **84** 062513
- [24] Hugi A, Villares G, Blaser S, Liu H C and Faist J 2012 Mid-infrared frequency comb based on a quantum cascade laser *Nature* **492** 229–33
- [25] Coluccelli N, Gambetta A, Sala T, Gatti D, Marangoni M, Laporta P and Galzerano G 2012 Frequency-stabilized 1 W optical comb at 2.2–2.6 μm by Cr²⁺:ZnSe multipass amplification *Opt. Lett.* **37** 4440–2
- [26] Gambetta A, Coluccelli N, Cassinerio M, Gatti D, Laporta P, Galzerano G and Marangoni M 2013 Milliwatt-level frequency combs in the 8–14 μm range via difference frequency generation from an Er: fiber oscillator *Opt. Lett.* **38** 1155–7
- [27] Jiang H *et al* 2008 Long-distance frequency transfer over an urban fiber link using optical phase stabilization *J. Opt. Soc. Am. B* **25** 2029–35
- [28] Zhang W, Lours M, Fischer M, Holzwarth R, Santarelli G and Le Coq Y 2012 Characterizing a fiber-based frequency comb with electro-optic modulator *IEEE Trans. Ultrason. Ferroelectr. Freq. Control* **59** 432–8
- [29] Chambon D, Bize S, Lours M, Narbonneau F, Marion H, Clairon A, Santarelli G, Luiten A and Tobar M 2005 Design and realization of a flywheel oscillator for advanced time and frequency metrology *Rev. Sci. Instrum.* **76** 094704
- [30] Guena J *et al* 2012 Progress in atomic fountains at LNE-SYRTE *IEEE Trans. Ultrason. Ferroelectr. Freq. Control* **59** 391–410

- [31] Chardonnet C and Bordé C J 1994 Hyperfine interactions in the ν_3 band of osmium tetroxide: accurate determination of the spin-rotation constant by crossover resonance spectroscopy *J. Mol. Spectrosc.* **167** 71–98
- [32] Acef O, Michaud F and Rovera G D 1999 Accurate determination of OsO₄ absolute frequency grid at 28/29 THz *IEEE Trans. Instrum. Meas.* **48** 567–70
- [33] Elliott D S, Roy R and Smith S J 1982 Extracavity laser band-shape and bandwidth modification *Phys. Rev. A* **26** 12–8
- [34] Kessler T, Hagemann C, Grebing C, Legero T, Sterr U, Riehle F, Martin M J, Chen L and Ye J 2012 A sub-40-mHz-linewidth laser based on a silicon single-crystal optical cavity *Nature Photon.* **6** 687–92
- [35] Eyres L A, Tourreau P J, Pinguet T J, Ebert C B, Harris J S, Fejer M M, Becouarn L, Gerard B and Lallier E 2001 All-epitaxial fabrication of thick, orientation-patterned GaAs films for nonlinear optical frequency conversion *Appl. Phys. Lett.* **79** 904
- [36] Yao Y, Hoffman A J and Gmachl C F 2012 Mid-infrared quantum cascade lasers *Nature Photon.* **6** 432–9